

Request Form for Translation

Translation Branch
The world of foreign prior art to you.

Translations

U. S. Serial No. : 09/712,596

Requester's Name: HAL WACHSMAN

Phone No. : 203-305-9288

Fax No. : _____

Office Location: CP4-8804

Art Unit/Org. : 402803

Group Director: Howard Goldberg

Is this for Board of Patent Appeals? _____

PTO 2002-3952

S.T.I.C. Translations Branch

Foreign Patents

Date of Request: 7-26-02

Date Needed By: 7-30-02

(Please do not write ASAP-indicate a specific date)

Phone: 308-0881
Fax: 308-0989
Location: Crystal Plaza 3/4
Room 2C01

SPE Signature Required for RUSH: Maur Hoff

Document Identification (Select One):

(Note: Please attach a complete, legible copy of the document to be translated to this form)

1. ☒ Patent

Document No. DE 195 21387 A1

Language German

Country Code DE

Publication Date 12-14-96

_____ (filled by STIC)

2. ☐ Article

Author _____

Language _____

Country _____

3. ☐ Other

Type of Document _____

Country _____

Language _____

Document Delivery (Select Preference):

_____ Delivery to nearest EIC/Office Date: 7-31-02 (STIC Only)

_____ Call for Pick-up Date: _____ (STIC Only)

_____ Fax Back Date: _____ (STIC Only)

To assist us in providing the most cost effective service, please answer these questions:

Will you accept an English Language Equivalent?
Yes (Yes/No)

Will you accept an English abstract?
No (Yes/No)

Would you like a consultation with a translator to review the document prior to having a complete written translation?
No (Yes/No)

Check here if Machine Translation is not acceptable:
(It is the default for Japanese Patents, '93 and onwards with avg. 5 day turnaround after receipt)

STIC USE ONLY

Copy/Search

Processor: 11

Date assigned: 7-29

Date filled: 7-29

Equivalent found: _____ (Yes/No)

Doc. No.: _____

Country: _____

Remarks: _____

Translation

Date logged in: 7-29-02

PTO estimated words: 2113

Number of pages: 11

In-House Translation Available: _____

In-House: _____ Contractor: _____

Translator: mw Name: _____

Assigned: 7-29-02 Priority: _____

Returned: 7/31/02 Sent: _____

Returned: _____

MACHINE TRANSLATION FEEDBACK FORM

Please fill out this form after reviewing your machine translation and return to Translations Branch, STIC, CP3/4. This information will help us determine the effectiveness of providing machine translations.

Filling out this form is entirely voluntary, and all information will be used solely by the Translations Branch for information purposes.

1. How much time did you spend reviewing the machine translation?

2. Did you find what you were looking for in the machine translation, or did you also request an oral translation for clarification?

3. Did you find that having a machine translation saved you time?

4. Please provide any other comments or suggestions.

**STIC Translations Branch is now offering Machine Translated
Japanese Patent Documents to all Technology Centers**

- The advantage of machine translation is faster turnaround time and lower costs.
- Presently, machine translation is available for Japanese Unexamined A (Kokai) documents 1993 onward and Japanese Patent B documents 1994 and onwards.
- **When submitting your request for a Japanese document, it is important to clearly indicate if the requested document is an A or B document because the Japanese patent system reuses patent numbers.**
- The vendor is supplying machine translations which have been reviewed by language and art area experts. However, at times, the sentence structure and syntax of machine translations can be awkward. When in doubt, please call one of the STIC Japanese translators for clarification. Their contact information is included here.
- We will continue to check if an English-language equivalent is available prior to processing a request and encourage using it, when possible.
- The attachments below provide additional information about the process and the service.
- **Unless otherwise indicated, STIC will process requests from alt TC's which meet these guidelines, as machine translation requests.**

We welcome your feedback; included is an evaluation form which can be dropped off at the Translations Branch, or e-mailed to STIC-Translations Box.

John Graham
Branch Chief
Translations

Arti Shah
Division Chief
STIC

Kristin Vajs
Director
STIC

Attachments:

-Request Form:

-Machine Translation Information/Background:

-Internet Sites as Sources for Translations:

Note: Unexamined Japanese A (Kokai) documents can be viewed for free at the Japanese Web site: http://www.ipdl.jpo-miti.go.jp/homepg_e.ipdl. The translations are raw machine translations.

- Evaluation Form:

Translation Staff Information:

JOHN R. GRAHAM-Supervisor	- Room 103 - 308-3293
AKIKO SMITH	- Room 108 - 308-3244
JOHN M. KOYTCHOFF	- Room 106 - 308-1185
MARTHA WITEBSKY	- Room 104 - 308-3282
STEVEN SPAR	- Room 105 - 308-3281
MATTHEW ALT	- Room 109 - 305-3530
CHISATO MOROHASHI	- Room 107 - 308-3279

Guidelines for Use of Machine Translations of Japanese Patents


Machine translations are an excellent, cost effective, rapid way of determining the information presented in a patent and identifying patents which are relevant. It is the quickest way to determine the essence of a particular foreign language document, i.e. "gisting". Machine translation is often used as a tool to aid human indexers by saving time spent in terminology lookups.

Approximately 27% of the requests for translation received in STIC are for Japanese patents from 1993 onwards. A few vendors have started offering machine translation of Japanese patent documents. The pilot indicated this type of service can play a role in helping examiners determine the basic information in Japanese patent.

Machine translation will help control translation costs, will improve the timeliness of translations, and in most cases provide an adequate product. Some machine translated patents or parts of patents will require human oral or written translation at a later point.

The following information is provided as background. Please keep these points in mind when using machine translations.

- When one has numerous Japanese documents submitted by an applicant, the MT product may prove sufficient to determine the basic information when the examiner considers it necessary to do so. Machine translation is good for determining if certain concepts or words appear in the patent and in providing an overall look at the content of the patent. STIC does not recommend its use in a court of law, unless consultation with a STIC translator has taken place.
- The meanings of words can be context-bound and the syntax is not always clear in machine translated text. The translated sentence structure may be confusing to interpret. The qualities of translations are good from the standpoint of terminology; grammar is often weak, but improving. When in doubt, a translator should be contacted. When a response to a rejection raises questions about the content of a foreign reference, the examiner should obtain at least a partial written translation of the portions in question.
- Any portion of a reference relied upon for a final rejection or appeal should be confirmed by a human translator, even if it is only a confirmation by a human translator of the accuracy of the MT translation. The confirmed translation of a disputed portion should preferably be included in the next office action.
- We will be using Human Assisted Machine Translations (MATS). MATS are an automated translation of text, using complex technology, from one natural language to another, by a computer. The translation is reviewed by human translators. The MAT gives a quick idea of the content of the patent document, is cost effective and offers a quicker turnaround. The pilot vendor, Derwent promises 5-day turnaround time from the point their Japanese Office receives the request. STIC monitors their performance. Requests are transmitted to the Derwent US office by STIC after initial processing.
- The format of the machine translated documents provided -two columns of the original Japanese text and the English translation-is designed to facilitate the accurate selection of content for follow-up custom translation.

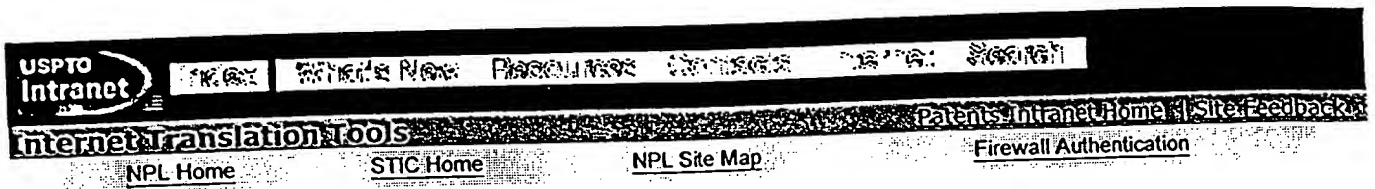

STIC TRANSLATIONS BRANCH

Internet Translation Tools

There are many tools available over the Internet which may be useful to you when you need a quick answer to the meaning of a particular word or phrase in a foreign language. Below you will find a list of Internet sites that are used as additional tools by some of the STIC translators and may be useful to you. However, caution should be exercised when using any of these tools. The specific subject matter and context in which a given term or expression is used will frequently determine how it should be translated into English. Most online dictionaries do not provide an adequate number of alternative translations for a given term or subject matter-specific examples of usage.

If you have any questions about this information, feel free to call the Translations Branch at 308-0881 or one of the translators on staff. To see a list of the translators, their background and experience as well as their phone numbers and location, [click here](#).

For technical translations for various languages:
<http://eurodic.ip.lu>

For non-technical terminology use:
<http://www.logos.it/dictionary>

A good source for multi-lingual glossary links with emphasis on German:
<http://www.jump.net/~fdietz/glossary.htm>

For German, French, Spanish, Portuguese and Italian:
<http://babelfish.altavista.com>

Another site for raw Machine Translations of Japanese Patents:
http://www.ipdl.jpo.go.jp/homepg_e.ipdl

Additional sites include:
<http://translate.dictionary.com/>
<http://www.dictionary.com/translate/>
<http://www.facstaff.bucknell.edu/rbeard/diction.html>

[USPTO Intranet Home](#) | [Index](#) | [What's New](#) | [Resources](#) | [Contacts](#) | [Internet](#) | [Search](#) | [Firewall](#) | [Web Services](#)

Last Modified: Wednesday, September 05, 2001 10:34:38

PTO 2002-3952

DE 19,521,387

Translation of German Patent Document No. 19,521,387

Inventor: Roland Gesche et al.

Applicant: Balzers und Leybold Deutschland Holding AG

Priority Date: N/A

Int. Class: H05 H 1/46; H03 H 7/40; G05 B 13/02

Application Date: June 13, 1995

Publication Date: December 19, 1996

Original German Title: Verfahren zum automatischen Abstimmen eines Anpassungsnetzwerks, das zwischen einer elektrischen Energiequelle und einer Last angeordnet ist.

METHOD FOR AUTOMATIC TUNING A MATCHING OR ADAPTOR
NETWORK ARRANGED BETWEEN AN ELECTRICAL POWER
SOURCE AND AN LOAD

Description

The invention relates to a method as defined in the preamble of Claim

1.

High frequency plasma generation in systems for the application and removal of thin layers has found wide acceptance. In this case, the variable impedance of the plasma must be transformed to the steady load impedance of a 13.56 Mhz high frequency generator and may be 50 Ohm. To accomplish this, matching or adaptor networks are commonly used which are arranged between the high frequency generator and the plasma path.

Such matching or adaptor networks are provided with variable coils and/or capacitors which are adjusted manually in order to do the matching.

Methods for controlling a plasma process are already known in which the change in impedance of a high frequency performance is indicated (US-A-4,207,137). In this case, an impedance recorder is configured as a phase and quantity detector. This recorder comprises inductive current recorders which can only be protected with great difficulty from capacitive couplings. Automatic matching cannot be accomplished by means of the impedance recorder.

In another known matching circuit for supplying high frequency electromagnetic power to a variable impedance, a plurality of tunable capacitors and tunable inductances are provided (US-A-4 679 007). In this case, the inductively operating recorders and phase analysers that are used are afflicted with drawbacks.

An automatic antenna coupler is also known which employs a system in which the real portion of a complex impedance or admittance is measured which is provided by an antenna or a network (US-A-3,913,644). In this case, an inductive current converter is used as measurement recorder.

An finally, a circuit arrangement for automatically tuning a matching network is known in which two electrical values are measured in the

matching network and are supplied to the control unit (DE-A-39 23 662).

The control unit employs these values to provide the total of three electrical values and, based on these values, it adjusts the inductance and/or capacitance of the matching network. This means that a high frequency generator is connected by a coaxial line to a matching network, a so-called "matchbox," with the cathode being connected to the output of the matchbox. At the input of the matching network a measurement recorder, for example, a phase-value detector, which generates two signals which contain information about the mismatch of the matchbox. These signals are supplied to the control unit which typically delivers the adjusted values to motor-adjustable capacitors of the matchbox. A drawback in this case is that the characteristic field of the match is a function of the load impedance, but matching the control strategy to the load impedance is not an option. This tends to cause the control to oscillate with some loads or to cause insufficient minimization. Sometimes it is necessary to repeat the adjustment for different loads, and this limits the flexibility. Previous controls have also tended to drift, and this is not always correctable by a new adjustment.

If mismatches occur, automatic tuning cannot find the adjustment range because, on the one hand, the characteristics of the mismatch range are

very complex and cannot be retraced by the controls and, on the other hand, the conventional records for mismatches are not sufficient to deliver sufficiently detailed two-dimensional information in the complex impedance field of the Smith diagram.

An active recorder with high dynamics and an improved control strategy, as known from the above-mentioned DE-A-39 23 662, is an improvement, but it is not a perfect solution, since the requirements on the load impedances constantly increase, especially if large cathodes are involved. Microcomputer-controlled controls cannot solve the problem alone without improved precision recorders.

It is therefore the object of the present invention to provide a stable matching circuit which is not afflicted with the aforementioned drawbacks.

The advantage obtained with the invention is more particularly that it is no longer necessary to employ high precision matching and, therefore, expensive recorders which cover the entire dynamic range. Nor is it necessary to undertake numerically extremely large control simulation which would only increase the uncertainty of the measurements.

An embodiment of the invention is described in greater detail below and illustrated in the drawing in which:

Fig. 1 is a view of a matching circuit for a variable load impedance including the associated control circuit;

Fig. 2 is an arrangement for generating the controlled values from the measured values.

Figure 1 illustrates a high frequency generator 1 which oscillates on a frequency of 13.56 MHz, and a matching network 2 connected to a variable load impedance 3. The matching network 2 is provided with three capacitors 3, 5, 6 in the longitudinal branch, and two parallel oscillating circuits 7, 8 in the transverse branch. These oscillating circuits 7, 8 are made of variable capacitors 9 and 10 and a stationary coil 11 and 12, with the oscillating circuit 8 being connected with one of its connectors to ground 13 and with the other connector between the capacitors 5 and 6, while the other oscillating circuit 7 is also connected to ground, but with the other connector it is connected to the capacitor 4 and 5.

Two different values are picked off the matching circuit 2 and fed to a control unit 14. These two values are the voltage U_E , which is present at the output of the high frequency generator, and the voltage U_1 , which is present at the parallel oscillating circuit 7. The voltages U_E and U_1 are fed by way of capacitive voltage distributors 15, 16, each of which contains two capacitors 17, 18 and 19, 20, to the control unit 14, which outputs control

values x_1 and x_2 . These control values x_1 and x_2 are amplified in amplifiers 21, 22 and are transmitted to adjustment motors 23, 24, which make an adjustment in the capacitors 9 and 10. The capacitors 9, 10, in this case, are adjusted in such a way that the matching network 2 always takes in a resistance value $Z_{E_{soll}}$, which corresponds to the inside resistance of the high frequency generator. When matching occurs, Z_E must be real and 50 Ohm. This determines the matching requirement for Z_{1soll} , i.e., the resistance value which must occur at U_1 up to 50 Ohm less the impedance of the stationary capacitor 4. Since this is very complex, the total of the two impedances make a statement about the real and imaginary portion of the reflection factor or the input impedance.

What is new, however, is that now the voltage is picked up from the output capacitors 6 and is fed via capacitors 46, 47 and 48, 49 to the control unit as signals $\sim U_1$ and $\sim U_2$.

Figure 2 illustrates the basic operation of the control unit 14 in greater detail. It can be seen that the signals,

$$\sim U_E \text{ and } \sim U_1$$

in this case, are each fed to a band pass filter 27, 28. The transmission functions of these filters 27, 28 and the transmission functions of the voltage distributor 15, 16, in this case, are in phase, which can be easily

accomplished by a corresponding adjustment. The output signals of the two band pass filters 27 and 28 are fed into a subtracter 26 to which a rectifier 29 is connected whose output signal is fed to two dividers 30, 31. The output signal of band pass filter 27 is further fed to a rectifier 32 whose output is connected to a second input of the dividers 30. The output signal of the band pass filter 28 also reaches a second input of the divider whose output signal is again fed to two control value generators 34 and 35. A third control value generator 36 only receives the output signal from the divider 30. The output signal of this control value generator 36 is applied to a normal amplifier 37 and an inverting amplifier 38 and from there it is fed to an output 39 or 40. The output signals of the control value generator 34, 35, however, are fed to outputs 40 or 39 via a PID-control unit 41 or 42. Control values x_1 , x_2 , which are fed to the adjustment motors 23, 24, are then present at outputs 39, 40, as illustrated in Fig. 1.

The signal $\sim U_A$ is fed via a band pass filter 50 and a rectifier 52 to a divider 54. A further signal $\sim U_2$ is fed via a band pass filter 51 and a rectifier 53 on a further divider 55.

Fuzzy logic is applied to the circuit arrangement in Fig. 1 and Fig. 2. In this case, fuzzy logic is involved which processes the truth values of a statement (linguistic variable) between 0 and 1. The number of the

“degrees of truth” is a function of the concrete realization. Both analogue (continuous) and multiple value digital (quantitized) realizations are available in this case. The most important basic operators of the fuzzy logic are the fuzzy-AND (minimum operator) and the fuzzy OR (maximum operator) and the fuzzy-NOT (negation). Although the minimum operator always forms the minimum of the degrees of truth of a plurality of variables, for example, $\text{MIN}(0.5; 0.8; 0.2) = 0.2$. The limiting case in binary logic is $\text{AND}(0; 1) = \text{MIN}(0; 1) = 0$. The maximum operator always forms the maximum degree of truth of a plurality of variables, for example, $\text{MAX}(0.5; 0.8; 0.2) = 0.8$. The limiting case in binary logic is the OR $(0; 1) = \text{MAX}(0; 1) = 1$. However, for final sequencing or processing fuzzified values (variables), the AND is often not optimal, since in minimum formation it does not take into consideration other points of view that occur at a slightly greater degree of truth and which would result in a certain compensation of the statement. This is why the compensatory AND (gamma operator) was also introduced. Selecting a parameter γ ($0 < \gamma < 1$) allows for an operator to be set continuously from a minimum operator ($\gamma = 0$) to a maximum operator ($\gamma = 1$). The fuzzy negation is simply the complement formation ($F' = 1 - F$) of fuzzy variables. The negation of the binary logic is included here too as a limiting case ($\text{NOT}(0) = 1 = 1 - 0 = 1$ or $\text{NOT}(1) = 1 - 1 = 0$).

The basic principle of processing this unclear data is product rule

IF... THEN. The application of fuzzy logic can result in more optimal system concepts or system solutions, for example, in control technology, since unclear statements often correspond better to the truth than the binary statement "true" (1) or "false" (0).

Three strategies are superimposed in this type of fuzzy logic system:

1. Measurement of the plasma impedance, calculation of the required capacity value, adjustment of the capacitors (reliable in case of mismatch, fast, but not precise);

2. Measurement of the matchbox input impedance, formation of the G' adjustment signals from the deviation in calibration (precise in case of a good match, poor capture behavior in case of a mismatch);

3. Minimization of the generator-Pr indicator (difficult automatically, but required for the calibration).

As a consequence, the control is an uncertain system. First, three independent strategies are formed, which are partially more based on empirical statements and partially on simplified system descriptions. The statements of these strategies must be suitably superimposed. Case differentiation and commutation are out of the question, since this would lead to instabilities and oscillation, because the different strategies may be

completely contradictory. In this case, a fuzzy control system is employed. This allows dependable behavior to be realized if all individual information is unstable but redundancy is available for all. The different strategies are formulated in fuzzy syntax and applied in parallel.

Claims

1. Method for the automatic tuning of a matching network, which is arranged between an electric power source and a load, characterized in that an automatic tuning control unit is used which operates as a fuzzy system.

2. Method as defined in Claim 1, characterized in that the load is a plasma path, that the impedance of this plasma path is measured, the capacity of the capacitor of the matching network is calculated based on the measurement of the plasma impedance and is adjusted correspondingly.

3. Method as defined in Claim 1, characterized in that the input impedance of the matching network is measured and if there is a deviation in the input impedance of a predetermined value, an adjustment signal is determined for the capacitors of the matching network, and the capacitor or capacitors are adjusted correspondingly.

4. Method as defined in Claim 1, characterized in that the wattage of the power source is minimized.

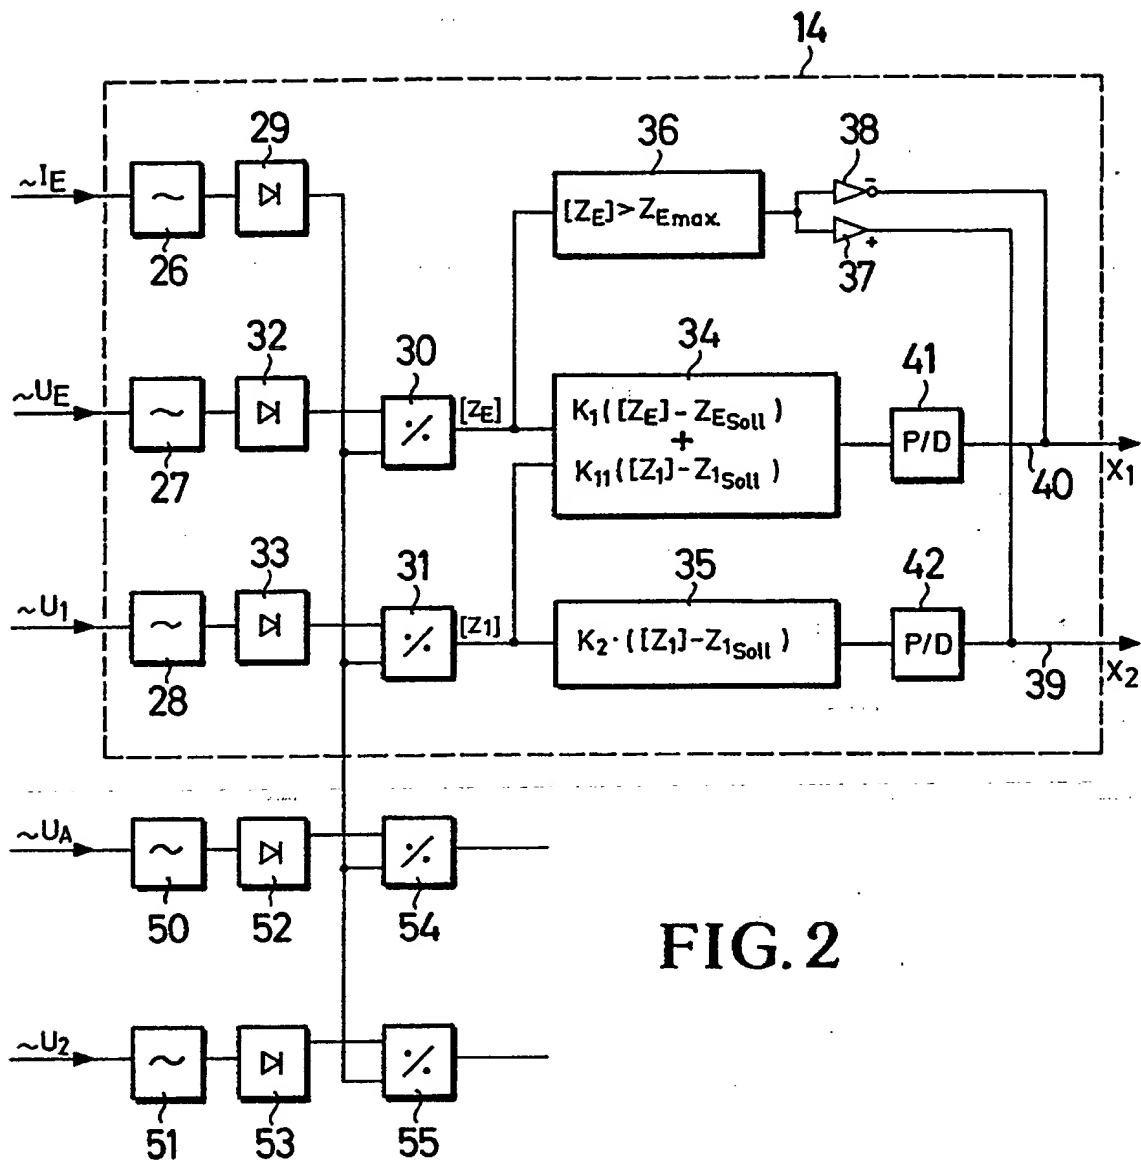


FIG. 2

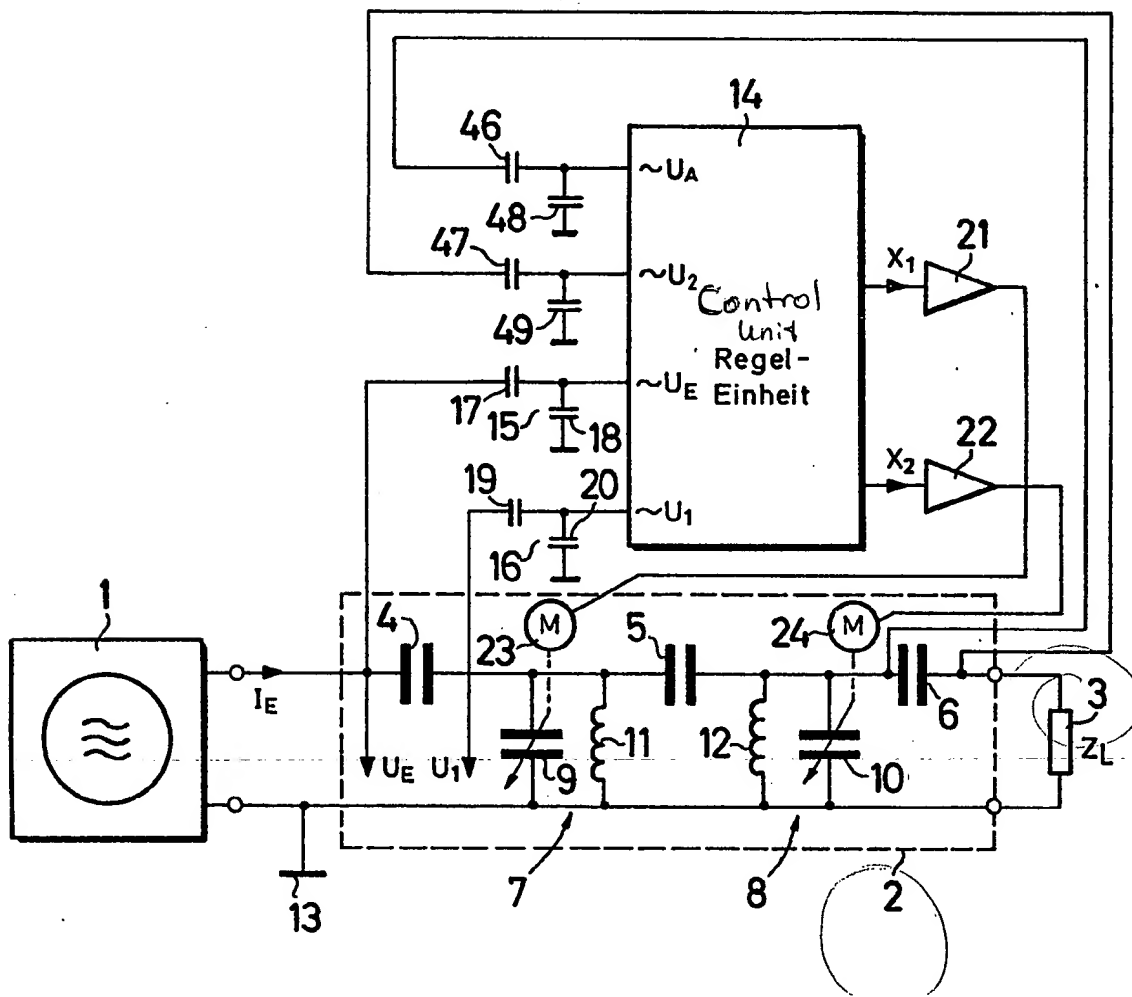


FIG.1 *

5. Method as defined in Claims 2 to 4, characterized in that the three methods are superimposed in a fuzzy system.

6. Method as defined in Claims 4, characterized in that subsequent to minimizing of the wattage of the power source, a calibration of the matching network occurs.

US Patent and Trademark Office
Translations Branch
Martha Witebsky - July 30, 2002